Biological indicator process challenge device (BI PCD)
or "BI test pack"

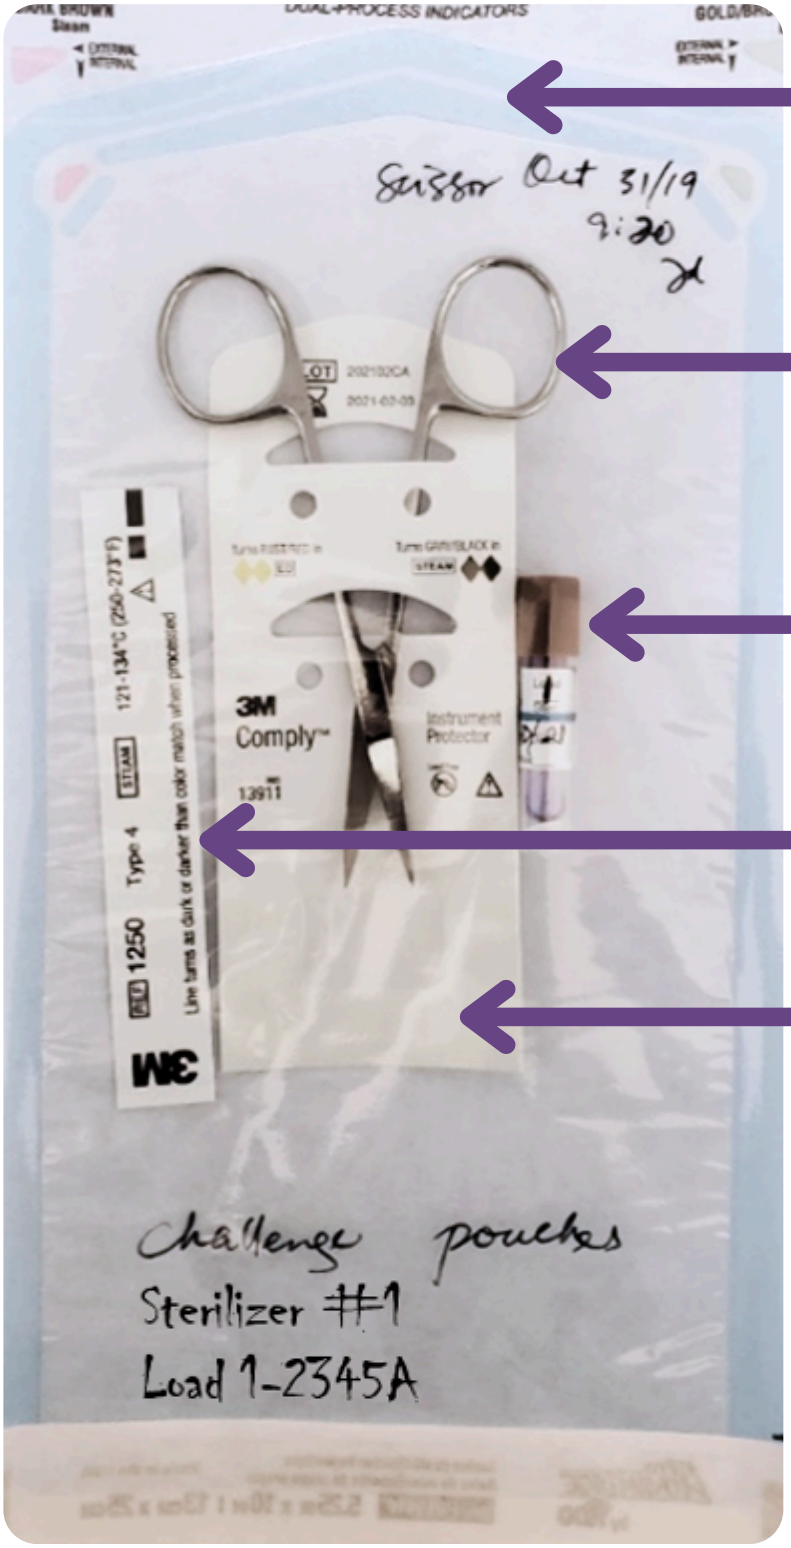

A Packaging (peel pouch, wrap)

B Largest/bulkiest instrument(s) to be sterilized

C Biological indicator (BI)

D Internal chemical indicator (CI)

E Other accessories (tip protector, instrument guard)

QUESTIONS?

Contact the CPSA IPAC Program at ipac@cpsa.ab.ca or 780-969-5001